

**LOCTITE®**



# **LOCTITE® 3D MED413™**

HDT60 Tough  
Clear, White

**LOCTITE®**

Henkel Corporation

[loctite3dp@henkel.com](mailto:loctite3dp@henkel.com)



**MED413™**  
HDT60 TOUGH  
CLEAR, WHITE



## LOCTITE 3D MED413™

LOCTITE 3D MED413 is a high-performance, high modulus material with excellent flexural and tensile physical properties. Stiffness combined with toughness make this material ideal for use in a wide variety of impact resistant medical device applications.

LOCTITE 3D MED413 is capable of meeting ISO 10993-5, -10 and -23 standards for biocompatibility when processed using a validated workflow. Certificates of Compliance are available upon request.

LOCTITE 3D MED413 is compatible with a broad range of DLP machines.



### Benefits:

- Capable of meeting ISO 10993-5 & -10 standards for biocompatibility
- Parts can function at body temperature
- Outstanding surface finish
- Excellent machineability



### Ideal for:

- Medical devices
- Hearing Aids
- Medical equipment components



### Markets:



### Healthcare

Tensile Stress at Break (MPa)

40

Young's Modulus (MPa)

1600

Elongation at Break (%)

50

HDT at 0.455 MPa (°C)

70

*\*Values shown are linked to LOCTITE MED413 CLEAR as reference, please refer to the specific mechanical properties for each of the colors shown in this document*



## PROPERTIES

Mechanical Properties	Measure	Method	Green	Post Processed
Tensile Stress at Break	MPa	ASTM D638	30 - 34 <sup>[1]</sup>	40 - 48 <sup>[4]</sup>
Tensile Stress at Yield	MPa	ASTM D638	32 - 38 <sup>[1]</sup>	43 - 49 <sup>[4]</sup>
Young's Modulus	MPa	ASTM D638	1350 - 1450 <sup>[1]</sup>	1600 - 1750 <sup>[4]</sup>
Elongation at Break	%	ASTM D638	54 - 68 <sup>[1]</sup>	40 - 55 <sup>[4]</sup>
Flexural Modulus	MPa	ASTM D790	-	1500 - 1600 <sup>[5]</sup>
Flexural Strain at Break	%	ASTM D790	-	>5 <sup>[5]</sup>
IZOD Impact (Notched)	J/m	ASTM D256	-	50 - 65 <sup>[8]</sup>
HDT at 0.455 MPa	°C	ASTM D648	-	66 - 70 <sup>[9]</sup>
HDT at 1.82 MPa	°C	ASTM D648	-	52 - 54 <sup>[9]</sup>
Shore Hardness (5s)	D	ASTM D2240	-	76 <sup>[10]</sup>
Water Absorption (24 hr)	%	ASTM D570	-	2.7 - 2.8 <sup>[11]</sup>
<b>Other Properties</b>				
Solid Density	g/cm <sup>3</sup>	ASTM D1475	1.2 <sup>[2]</sup>	1.2 <sup>[2]</sup>
<b>Biocompatibility</b>				
Cytotoxicity		ISO 10993-5	-	Comply <sup>[6]</sup>
Sensitization		ISO 10993-10	-	Comply <sup>[7]</sup>
Irritation		ISO 10993-23*	-	Comply <sup>[12]</sup>
<b>Liquid Properties</b>				
Viscosity	cP	ASTM D7867		500-600 <sup>[3]</sup>
Liquid Density	g/cm <sup>3</sup>	ASTM D1475		1.1 <sup>[2]</sup>

\*All the properties above are specific to a validated workflow using an Origin One printer and Dymax 5000-EC post-cure unit. Deviations from this workflow may lead to deviations in the properties. All specimen are printed unless otherwise noted. All specimen were conditioned in ambient lab conditions at 19-23°C / 40-60% RH for at least 24 hours. ASTM Methods: D638 Type IV, 15 mm/min, D790-B, 2 mm/min, D648, D256 Notched IZOD (notched after post-cure), 6 mm x 12 mm, D570 0.125" x 2" Disc 24hr@ 25°C, D2240, Type "D" (0, 3 seconds), D7867, D1475

\*The biological assessment has been performed based on the in vitro method according to ISO10993-23

**Internal Data Sources:**

[1] FOR25854/FOR27583/FOR36108, [2] FOR36096, [3] FOR34279, [4] FOR27584/FOR30160/FOR36105, [5] FOR36104, [6] FOR19950, [7] FOR21402, [8] FOR36117, [9] FOR36121, [10] FOR36122, [11] FOR36128, [12]FOR52784(in vitro)



**MED413™**  
HDT60 TOUGH  
CLEAR



## WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

### PRINTER SETTINGS

LOCTITE 3D MED413 CL is formulated to print optimally on industrial DLP printer. Read the safety data sheet carefully to get details about health and safety instructions. Recommended print parameters:

- Shake resin bottle well before usage
- Temperature: 20°C to 25°C
- Intensity: 4 mW/cm<sup>2</sup> to 8 mW/cm<sup>2</sup>

#### Exposure time for an intensity of 5 mW/cm<sup>2</sup>

Layer Thickness (µm):	100	E <sub>c</sub> (mJ/cm <sup>2</sup> )	10.31
First layer time (s)	15	D <sub>p</sub> (mm):	0.27
Burn in region (s):	8		
Model Layer Exposure (s):	5		

### CLEANING

LOCTITE 3D MED413 CL requires post processing to achieve specified properties. Prior to post curing, support structures should be removed from the printed part, and the part should then be washed. Use compressed air to remove residual solvent from the surface of the material between intervals.

Post Process Step	Agent	Method	Duration	Intervals	Additional Info
Cleaning Cycle 1	IPA	Ultra sonic bath	2 min	1	Allow parts to dry between intervals
Cleaning Cycle 2	IPA	Ultra sonic bath	2 min	1	Use fresh IPA
Dry	n.a.	Compressed air	10 to 60 s	2	Air pressure (30psi)
Wait before post curing	n.a.	Ambient condition	60 min	1	Room temperature



**MED413™**  
HDT60 TOUGH  
CLEAR



## WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

## POST CURING

**LOCTITE 3D MED413 CL** requires post curing to achieve specified properties. It is recommended that either an LED or wide spectrum lamp be used to post cure parts.

UV Curing Unit	UV Source	Intensity	Cure time/ side	Additional Settings (Shelf, Output Energy)
Dymax 5000 EC Flood	Mercury Arc Bulb (broad spectrum)	150 mW/cm <sup>2</sup> at 380 nm	4 min	Shelf K
Loctite UVALOC 1000	Mercury Arc Bulb (broad spectrum)	30 mW/cm <sup>2</sup> at 365 nm	5 min	500 W, 3rd shelf from bottom
Loctite CL36	405nm LED	80 mW/cm <sup>2</sup> at 405 nm	30 min	100% top & side

## STORAGE

Store **LOCTITE 3D MED413 CL** in the unopened container in a dry location. Optimal Storage: 8°C to 30°. Storage below 8°C or above 30°C can adversely affect product properties. Material removed from containers may be contaminated during use. For this reason, filter used resin with 190µm mesh filter before placing back into proper storage container.







**MED413™**  
HDT60 TOUGH  
CLEAR



## AGEING AND ENVIRONMENTAL EFFECTS – HEAT AGEING

LOCTITE 3D MED413 CL was heat aged without load according to ASTM D3045. Test samples were exposed for a defined time at 50°C and conditioned for 24 hours at 22°C before mechanical testing. Control samples were stored at a constant 22°C. All samples were printed in the same print job using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C). "0 weeks" represents non-aged samples stored at 22°C and tested 24 hours after post-processing.

Based on temperature dependence of reaction rates a test time of 6 weeks at 50°C can be interpreted as approximately 12 months at ambient temperature.

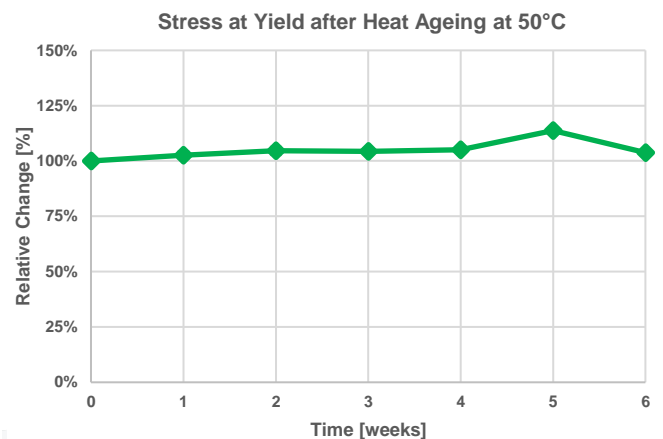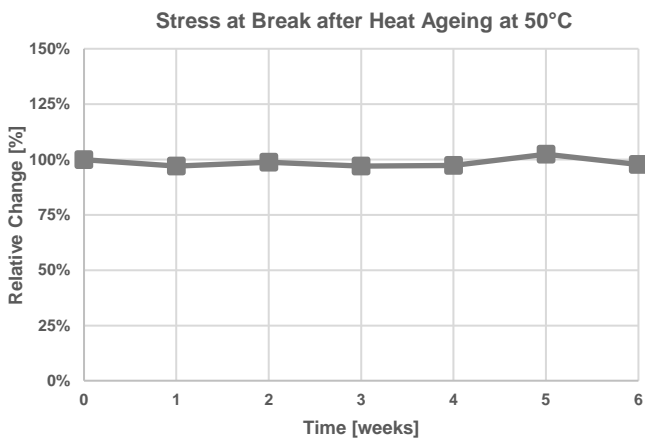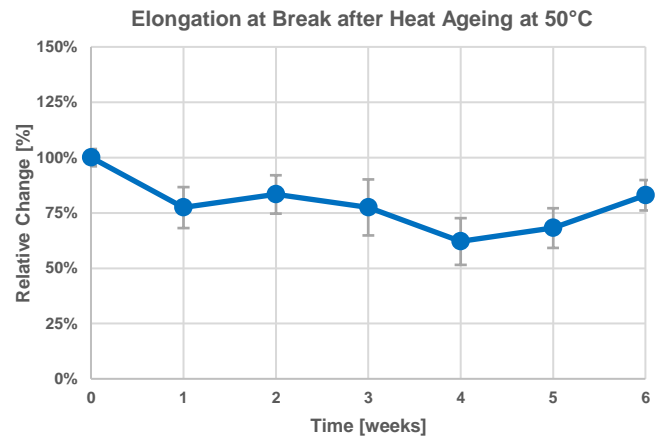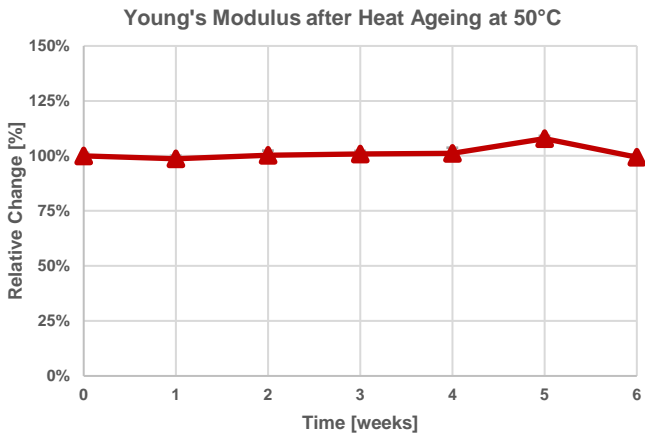

**Test parameters:**

ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1.0% (regression), 22°C

**Internal Data Sources:**  
FOR116848, FOR116849




**MED413™**  
HDT60 TOUGH  
CLEAR



## AGEING AND ENVIRONMENTAL EFFECTS – ACCELERATED WEATHERING (UV AGEING)

LOCTITE 3D MED413 CL has been tested after accelerated outdoor weathering according to ASTM D4329 (Cycle A). Test samples were exposed to defined conditions of heat, water condensation and UV light. Exposed samples were conditioned for 24 hours at 22°C before mechanical testing. Control samples were stored at a constant 22°C. All samples were printed in the same print job using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C). "0 weeks" represents non-aged samples stored at 22°C and tested 24 hours after post-processing.

Please note, accelerated weathering testing can never fully represent real outdoor conditions and complexity. It is therefore recommended to conduct additional (outdoor) testing relevant for your specific application needs.

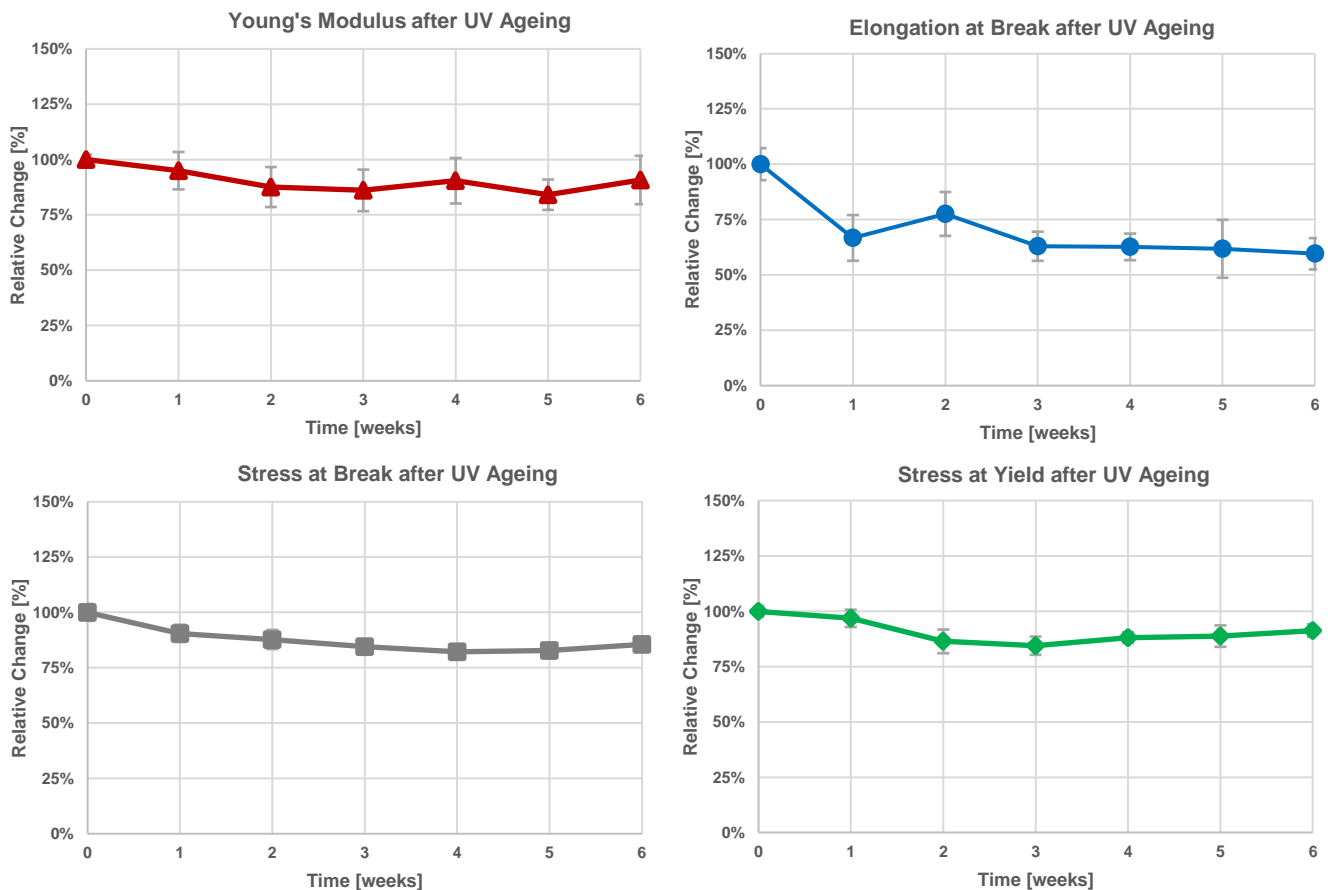

### Test parameters:

ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1% (regression), 22 °C  
ASTM D4329: cycle A for general applications, QUV/se, UVA 340 nm, 0.89 W/m<sup>2</sup>-nm, 8 hours UV light at 60°C followed by 4 hours at 50°C condensation in the dark. To reduce any sample warpage during test time samples were placed in tailor-made holders without any fixation clamps or mechanical load. Exposed samples were always removed from QUV before next condensation cycle to avoid samples that are soaked excessively with water before testing.

Internal Data Sources:  
FOR167570, FOR167584



**MED413™**  
HDT60 TOUGH  
CLEAR




## PHYSICAL PROPERTIES OF STERILIZED PARTS

ASTM D638 Type IV dog bones were printed with **LOCTITE 3D MED413 CL** and sterilized with autoclave steam and Ethylene Oxide sterilization processes. Each sterilization method had a sample set of n=8. Test samples were tested 24 hours after sterilization and compared to a control sample set of n=8.


### Autoclave Steam Sterilization: 134°C (270°F)

The tensile results of the sterilized dog bones parts show that the average Elongation at Break, Stress at Yield, and Young's Modulus values were outside the standard deviation of the non-sterilized control samples. After one cycle of 134°C steam sterilization, there is an effect to Elongation at Break, Stress at Yield, and Young's Modulus.

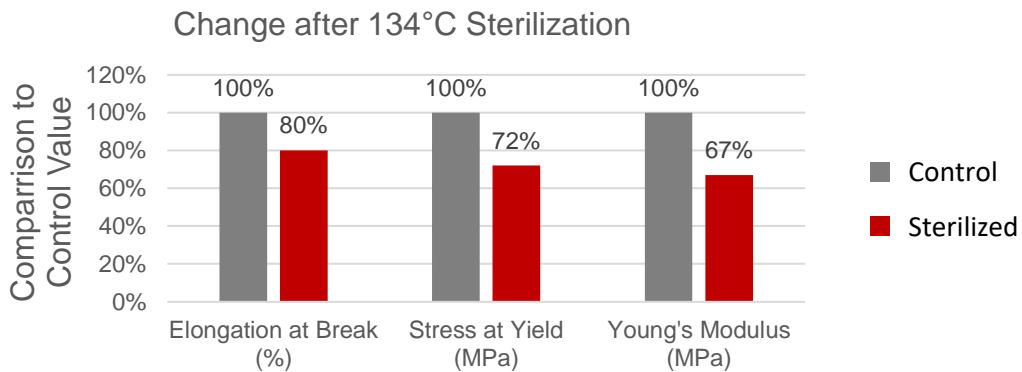

### Autoclave Steam Sterilization: 121°C (250°F)

The tensile results of the sterilized dog bones parts show that the average Elongation at Break, Stress at Yield, and Young's Modulus values were outside the standard deviation of the non-sterilized control samples. After one cycle of 121°C sterilization, there is an effect to Elongation at Break, Stress at Yield, and Young's Modulus.

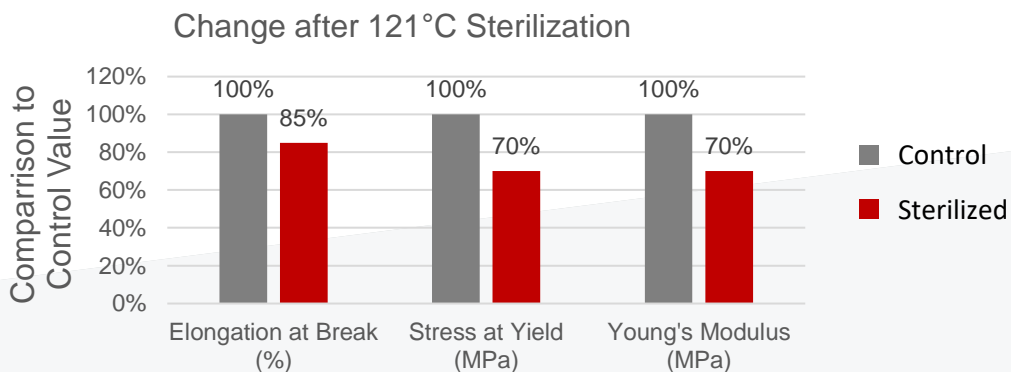






**MED413™**  
HDT60 TOUGH  
CLEAR



## PHYSICAL PROPERTIES OF STERILIZED PARTS


### Autoclave Steam Sterilization: 121°C (250°F) Extended Drying

The tensile results of the sterilized dog bones parts show that the average Elongation at Break, Stress at Yield, and Young's Modulus values were outside the standard deviation of the non-sterilized control samples. After one cycle of 121°C extended drying steam sterilization, there is an effect to Elongation at Break, Stress at Yield, and Young's Modulus.

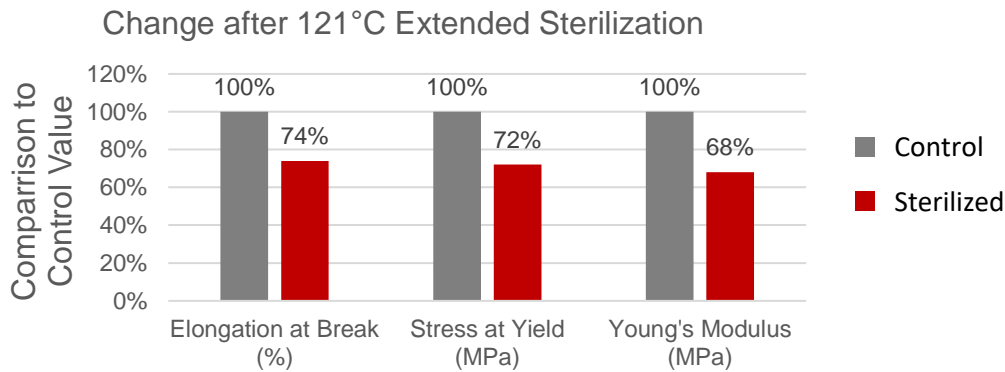

### Ethylene Oxide (EtO) Sterilization

The tensile results of the sterilized dog bones parts showed that the average Elongation at Break and Young's Modulus values were within the standard deviation of the non-sterilized control samples. The average Stress at Yield value of the sterilized samples was outside the standard deviation of the non-sterilized control samples. After one cycle of Ethylene Oxide sterilization, there is no significant effect to Elongation at Break, Stress at Yield, or Young's Modulus.

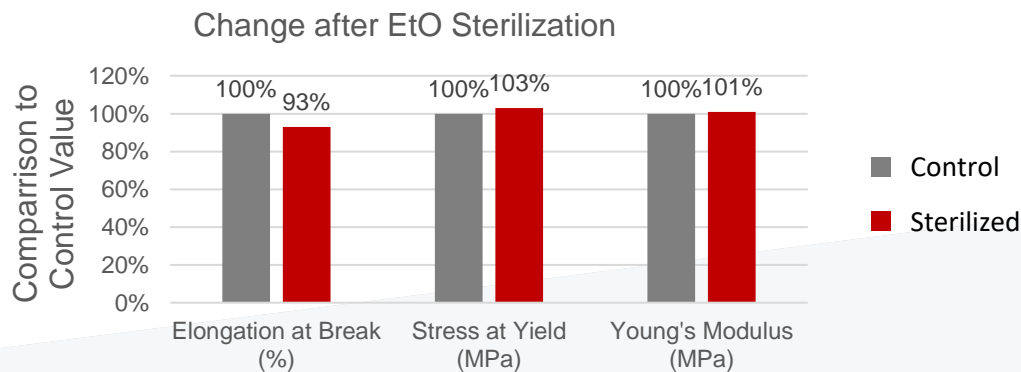



### PROPERTIES

Mechanical Properties	Measure	Method	Green	Post Processed
Tensile Stress at Break	MPa	ASTM D638	32 - 36 <sup>[1]</sup>	41 - 44 <sup>[4]</sup>
Tensile Stress at Yield	MPa	ASTM D638	37 - 40 <sup>[1]</sup>	45 - 47 <sup>[4]</sup>
Young's Modulus	MPa	ASTM D638	1500 - 1600 <sup>[1]</sup>	1650 - 1800 <sup>[4]</sup>
Elongation at Break	%	ASTM D638	60 - 75 <sup>[1]</sup>	47 - 55 <sup>[4]</sup>
Flexural Modulus	MPa	ASTM D790	-	1400 - 1600 <sup>[5]</sup>
Flexural Strain at Break	%	ASTM D790	-	>5 <sup>[5]</sup>
IZOD Impact (Notched)	J/m	ASTM D256	-	48 - 58 <sup>[8]</sup>
HDT at 0.455 MPa	°C	ASTM D648	-	68 - 69 <sup>[9]</sup>
HDT at 1.82 MPa	°C	ASTM D648	-	53 - 55 <sup>[9]</sup>
Shore Hardness (5s)	D	ASTM D2240	-	72 <sup>[10]</sup>
Water Absorption (24 hr)	%	ASTM D570	-	1 - 2 <sup>[11]</sup>
<b>Other Properties</b>				
Solid Density	g/cm <sup>3</sup>	ASTM D1475	1.2 <sup>[2]</sup>	1.0 <sup>[2]</sup>
<b>Biocompatibility</b>				
Cytotoxicity		ISO 10993-5	-	Comply <sup>[6]</sup>
Sensitization		ISO 10993-10	-	Comply <sup>[7]</sup>
Irritation		ISO 10993-23	-	Comply <sup>[12]</sup>
<b>Liquid Properties</b>				
Viscosity	cP	ASTM D7867		525-625 <sup>[3]</sup>
Liquid Density	g/cm <sup>3</sup>	ASTM D1475		1.1 <sup>[2]</sup>

\*All the properties above are specific to a validated workflow using an Origin One printer and Dymax 5000-EC post-cure unit. Deviations from this workflow may lead to deviations in the properties. All specimen are printed unless otherwise noted. All specimen were conditioned in ambient lab conditions at 19-23°C / 40-60% RH for at least 24 hours.\* ASTM Methods: D638 Type IV, 15 mm/min, D790-B, 2 mm/min, D648, D256 Notched IZOD (notched after post-cure), 6 mm x 12 mm, D570 0.125" x 2" Disc 24hr@ 25°C, D2240, Type "D" (0, 3 seconds), D7867, D1475

\*The biological assessment has been performed based on the in vitro method according to ISO10993-23

**Internal Data Sources:**

[1] FOR27567/FOR38326, [2] FOR38325, [3] FOR30596, [4] FOR28603/FOR38327, [5] FOR27825/38324, [6] FOR38849, [7] FOR21402, [8] FOR38323/FOR25330, [9] FOR38322, [10] FOR38321, [11] FOR38320, [12]52784 (in vitro)



## WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

## PRINTER SETTINGS

LOCTITE 3D MED413 WH is formulated to print optimally on industrial DLP printer. Read the safety data sheet carefully to get details about health and safety instructions. Recommended print parameters:

- Shake resin bottle well before usage
- Temperature: 20°C to 25°C
- Intensity: 4 mW/cm<sup>2</sup> to 8 mW/cm<sup>2</sup>

### Exposure time for an intensity of 5 mW/cm<sup>2</sup>

Layer Thickness (µm):	100	E <sub>c</sub> (mJ/cm <sup>2</sup> )	6.28
First layer time (s)	10	D <sub>p</sub> (mm):	0.14
Burn in region (s):	6		
Model Layer Exposure (s):	7		

## CLEANING

LOCTITE 3D MED413 WH requires post processing to achieve specified properties. Prior to post curing, support structures should be removed from the printed part, and the part should then be washed. Use compressed air to remove residual solvent from the surface of the material between intervals.

Post Process Step	Agent	Method	Duration	Intervals	Additional Info
Cleaning Cycle 1	IPA	Ultra sonic bath	2 min	1	Allow parts to dry between intervals
Cleaning Cycle 2	IPA	Ultra sonic bath	2 min	1	Use fresh IPA
Dry	n.a.	Compressed air	10 to 60 s	2	Air pressure (30psi)
Wait before post curing	n.a.	Ambient condition	60 min	1	Room temperature



**MED413™**  
HDT60 TOUGH  
WHITE



## WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

## POST CURING

**LOCTITE 3D MED413 WH** requires post curing to achieve specified properties. It is recommended that either an LED or wide spectrum lamp be used to post cure parts.

UV Curing Unit	UV Source	Intensity	Cure time/ side	Additional Settings (Shelf, Output Energy)
Dymax 5000 EC Flood	Mercury Arc Bulb (broad spectrum)	150 mW/cm <sup>2</sup> at 380 nm	4 min	Shelf K
Loctite UVALOC 1000	Mercury Arc Bulb (broad spectrum)	30 mW/cm <sup>2</sup> at 365 nm	2 min	500 W, 3 <sup>rd</sup> shelf from top
Uvitron Intelliray 600	Mercury Arc Bulb (broad spectrum)	130 mW/cm <sup>2</sup> at 380 nm	2 min	66% power, 3 <sup>rd</sup> shelf from top

## STORAGE

Store **LOCTITE 3D MED413 WH** in the unopened container in a dry location. Optimal Storage: 8°C to 30°. Storage below 8°C or above 30°C can adversely affect product properties. Material removed from containers may be contaminated during use. For this reason, filter used resin with 190µm mesh filter before placing back into proper storage container.



**MED413™**  
HDT60 TOUGH  
WHITE




## PHYSICAL PROPERTIES OF STERILIZED PARTS

ASTM D638 Type IV dog bones were printed with **LOCTITE 3D MED413 WH** and sterilized with autoclave steam and Ethylene Oxide sterilization processes. Each sterilization method had a sample set of n=8. Test samples were tested 24 hours after sterilization and compared to a control sample set of n=8.


### Autoclave Steam Sterilization: 134°C (270°F)

The tensile results of the sterilized dog bones parts show that the average Elongation at Break, Stress at Yield, and Young's Modulus values were outside the standard deviation of the non-sterilized control samples. After one cycle of 134°C steam sterilization, there is an effect to Elongation at Break and Young's Modulus, but no significant effect to Stress at Yield.

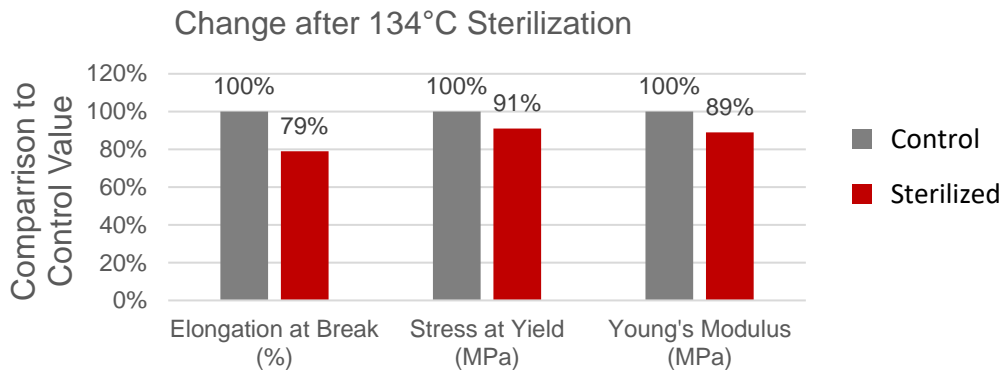

### Autoclave Steam Sterilization: 121°C (250°F)

The tensile results of the sterilized dog bones parts show that the average Elongation at Break, Stress at Yield, and Young's Modulus values were outside the standard deviation of the non-sterilized control samples. After one cycle of 121°C steam sterilization, there is an effect to Elongation at Break, Stress at Yield, and Young's Modulus.

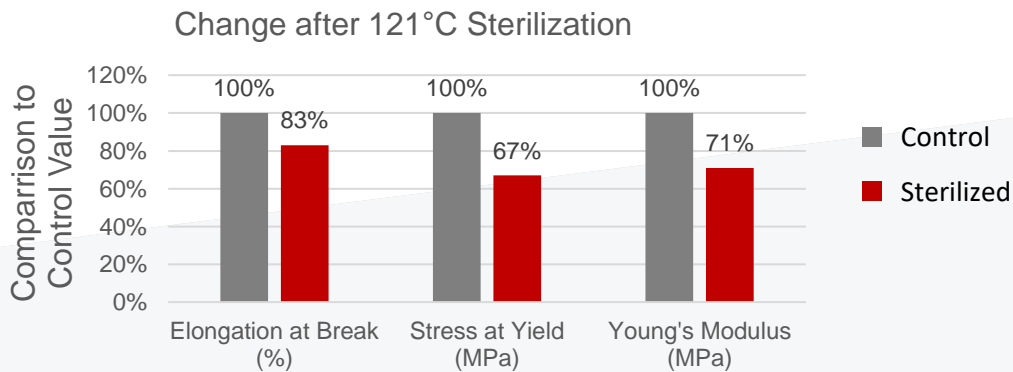




**MED413™**  
HDT60 TOUGH  
WHITE



## PHYSICAL PROPERTIES OF STERILIZED PARTS


### Autoclave Steam Sterilization: 121°C (250°F) Extended Drying

The tensile results of the sterilized dog bones parts show that the average Elongation at Break, Stress at Yield, and Young's Modulus values were outside the standard deviation of the non-sterilized control samples. After one cycle of 121°C extended drying steam sterilization, there is an effect to Elongation at Break, Stress at Yield, and Young's Modulus.

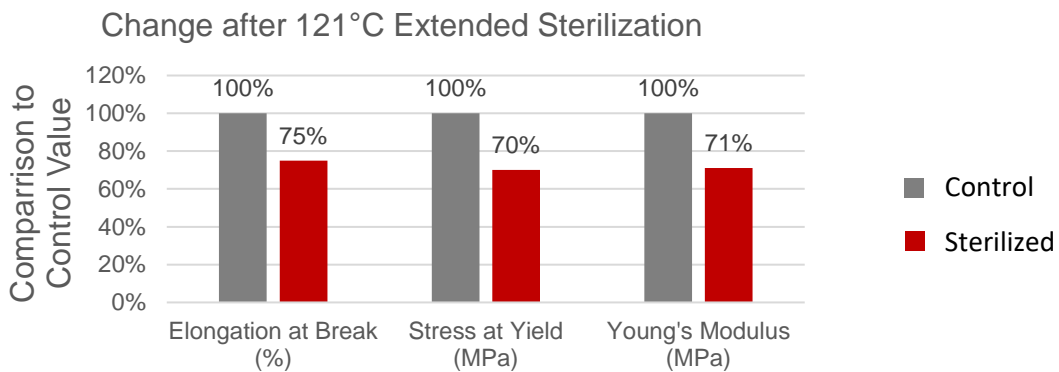

### Ethylene Oxide (EtO) Sterilization

The tensile results of the sterilized dog bones parts showed that the average Elongation at Break and Stress at Yield values were within the standard deviation of the non-sterilized control samples. The average Young's Modulus of the sterilized samples was outside the standard deviation of the non-sterilized control samples. After one cycle of Ethylene Oxide sterilization, there is no significant effect to Elongation at Break, Stress at Yield, or Young's Modulus.

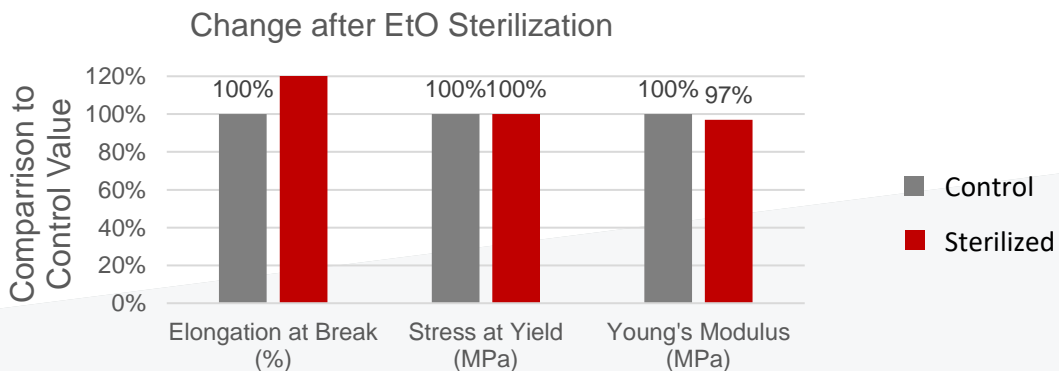



**MED413™**  
HDT60 TOUGH  
CLEAR, WHITE



## FURTHER INFORMATION REGARDING INSTRUCTIONS FOR USE

### OVERVIEW

**LOCTITE 3D MED413** is an energy-curable resin used to manufacture a variety of 3D printed biocompatible medical devices. Due to the physical properties and biocompatibility of the finished material, 3D printed parts can be used in a variety applications when processed in accordance with validated workflows. If sterile parts are required, please follow the guidance in this IFU to obtain an effective final device.

### Warnings and Precautions

When this product is used to create a Regulated Medical Device, either the user assumes all responsibility to use this product only for Henkel supported and approved Indications for use or the user must take all responsibility to register their indication of use with the proper regulatory authority. Strict adherence to our information for use and validated production workflows (printer, washing, and post processing procedures), is critical in assuring a safe, biocompatible and effective printed appliance.

Follow all recommended validated settings for safe and effective print results.

**LOCTITE 3D MED413** contains (meth)acrylate monomers and oligomers which, although rare, may cause an allergic reaction in individuals sensitive to acrylic containing products. Always review and understand all safety data sheets (SDS) and labels prior to use. Do not use any devices or components that have not been validated and deemed acceptable by Henkel. Parts must be printed and post processed in accordance with approved workflows prior to use. Always keep finished parts stored in a cool, dry place (15-30°C) and away from direct sunlight. Finished parts are not meant to be used for prolonged periods in outdoor environments.

Exact workflows with detailed information can be obtained by contacting us at [www.loctiteAM.com](http://www.loctiteAM.com).



**MED413™**  
HDT60 TOUGH  
CLEAR, WHITE



## DIRECTIONS FOR USE

1. Prior to printing, agitate the bottle of resin and allow the resin to adjust to an ambient temperature between 20-25°C / 68-77°F for a period of one hour.
2. Once the design is completed per CAD software manufacturers direction for use, import the CAM software unique to the printer manufacturer.
3. Nest the parts you would like to print in a CAM software.
4. Only print **LOCTITE 3D MED413** with the printer-specific pre-determined settings for DLP printers Henkel has validated. Contact us at [www.loctiteAM.com](http://www.loctiteAM.com) for validated printer settings. Alternative printers must be validated by Henkel to determine print settings needed to generate a safe and effective device.

## DIRECTIONS FOR POST-PROCESSING

1. When the print is complete, gently remove parts from the printer build platform and remove support structures from the part if applicable.
2. Wash the parts for the pre-determined duration and number of wash cycles. Henkel will have validated the workflow you will be using. Contact us at [www.loctiteAM.com](http://www.loctiteAM.com) for validated post-processing procedures.
3. Dry the parts with compressed air and inspect parts for any residual resin, which will have a glossy appearance. If any residual resin is observed, repeat step 2.
4. Allow the parts to rest at room temperature for 30-90 minutes before progressing.
5. Place parts in a single layer in a post-cure unit Henkel has validated and use the post-cure unit specific settings. Contact us at [www.loctiteAM.com](http://www.loctiteAM.com) for validated post-cure unit settings. Alternative post-cure units must be validated by Henkel to determine post-cure settings to generate a safe and effective device.





**MED413™**  
HDT60 TOUGH  
CLEAR, WHITE



## DIRECTIONS FOR STERILIZATION

LOCTITE 3D MED413 is suitable for sterilization using standards methods described below

### **Autoclave Steam Sterilization: 134°C (273°F)**

1. Samples should be packaged and distributed in the appropriate sterilization bags.
2. Bags should be laid flat and not stacked on top of one another to ensure adequate steam saturation.
3. Ramp temperature up to 134°C (273°F) and pressurize to 2.1 bar (30.5 psi) and hold for 4 minutes.
4. Depressurize chamber to -1.0 bar (-14.5 psi) and hold for a minimum of 5 minutes.
5. Temperatures may vary during the depressurization. If the temperature stays above 60°C in the depressurization phase, the finished parts will be in compliance.
6. Check that the bag sterilization confirmation marks are fulfilled and inspect parts for clarity. If parts are cloudy or opaque, parts were not dried completely and should not be used.

### **Autoclave Steam Sterilization: 121°C (250°F)**

1. Samples should be packaged and distributed in the appropriate sterilization bags.
2. Bags should be laid flat and not stacked on top of one another to ensure adequate steam saturation.
3. Ramp temperature up to 121°C (250°F) and pressurize to 1.1 bar (16.0 psi) and hold for 10 minutes.
4. Depressurize chamber from -0.7 (10.1 psi) to -1.0 bar (-14.5 psi) and hold for 5 minutes.
5. Temperatures may vary during the depressurization. If the temperature stays above 60°C in the depressurization phase, the finished parts will be in compliance.
6. Check that the bag sterilization confirmation marks are fulfilled and inspect parts for clarity. If parts are cloudy or opaque, parts were not dried completely and should not be used.



**MED413™**  
HDT60 TOUGH  
CLEAR, WHITE



## DIRECTIONS FOR STERILIZATION (CONTINUED)

### Autoclave Steam Sterilization: 121°C (250°F) Extended

1. Samples should be packaged and distributed in the appropriate sterilization bags.
2. Bags should be laid flat and not stacked on top of one another to ensure adequate steam saturation.
3. Ramp temperature up to 121°C (250°F) and pressurize to 1.1 bar (16.0 psi) and hold for 30 minutes.
4. Depressurize chamber from -0.7 (10.1 psi) to -1.0 bar (-14.5 psi) and hold for 60 minutes. Hold temperature at 97°C (207°F) during drying phase.
5. Temperatures may vary during the depressurization. If the temperature stays above 60°C in the depressurization phase, the finished parts will be in compliance.
6. Check that the bag sterilization confirmation marks are fulfilled and Inspect parts for clarity. If parts are cloudy or opaque, parts were not dried completely and should not be used.



**MED413™**  
HDT60 TOUGH  
CLEAR, WHITE



## STORAGE

Store **LOCTITE 3D MED413** in the unopened container in a dry location. Optimal storage: 8°C to 30°C, storage below 8°C or greater than 30°C can adversely affect products properties. More specific information is given in the Safety Data Sheet. Material removed from container may be contaminated during use. For this reason, filter used resin with 190µm mesh filter before placing back into proper storage container.

## BIOCOMPATIBILITY

Printed parts were prepared in accordance to the instructions provided in this document and submitted to an external lab for evaluation in accordance with ISO 10993-5, Biological evaluation of medical devices - Part 5: Tests for in vitro cytotoxicity.

When this product is used to create a Regulated Medical Device, either the user assumes all responsibility to use this product only for Henkel supported and approved Indications for use or the user must take all responsibility to register their indication of use with the proper regulatory authority. Strict adherence to our information for use and validated production workflows (printer, washing, and post processing procedures), is critical in assuring a safe, biocompatible and effective printed appliance.



**MED413™**  
HDT60 TOUGH  
CLEAR, WHITE



## NOTE

The information provided in this Technical Data Sheet (TDS) including the recommendations for use and application of the product are based on our knowledge and experience of the product as at the date of this TDS. The product can have a variety of different applications as well as differing application and working conditions in your environment that are beyond our control. Henkel is, therefore, not liable for the suitability of our product for the production processes and conditions in respect of which you use them, as well as the intended applications and results. We strongly recommend that you carry out your own prior trials to confirm such suitability of our product.

Any liability in respect of the information in the Technical Data Sheet or any other written or oral recommendation(s) regarding the concerned product is excluded, except if otherwise explicitly agreed and except in relation to death or personal injury caused by our negligence and any liability under any applicable mandatory product liability law.

In case products are delivered by Henkel Belgium NV, Henkel Electronic Materials NV, Henkel Nederland BV, Henkel Technologies France SAS and Henkel France SA please additionally note the following:

In case Henkel would be nevertheless held liable, on whatever legal ground, Henkel's liability will in no event exceed the amount of the concerned delivery.

In case products are delivered by Henkel Colombiana, S.A.S. the following disclaimer is applicable:

The information provided in this Technical Data Sheet (TDS) including the recommendations for use and application of the product are based on our knowledge and experience of the product as at the date of this TDS. Henkel is not liable for the suitability of our product for the production processes and conditions in respect of which you use them, as well as the intended applications and results. We strongly recommend that you carry out your own prior trials to confirm such suitability of our product.

Any liability in respect of the information in the Technical Data Sheet or any other written or oral recommendation(s) regarding the concerned product is excluded, except if otherwise explicitly agreed and except in relation to death or personal injury caused by our negligence and any liability under any applicable mandatory product liability law.

In case products are delivered by Henkel Corporation, Resin Technology Group, Inc., or Henkel Canada, Inc. the following disclaimer is applicable:

The data contained herein are furnished for information only and are believed to be reliable. We cannot assume responsibility for the results obtained by others over whose methods we have no control. It is the user's responsibility to determine suitability for the user's purpose of any production methods mentioned herein and to adopt such precautions as may be advisable for the protection of property and of persons against any hazards that may be involved in the handling and use thereof. In light of the foregoing, Henkel Corporation specifically disclaims all warranties expressed or implied, including warranties of merchantability or fitness for a particular purpose, arising from sale or use of **Henkel Corporation's products. Henkel Corporation specifically disclaims any liability for consequential or incidental damages of any kind, including lost profits.** The discussion herein of various processes or compositions is not to be interpreted as representation that they are free from domination of patents owned by others or as a license under any Henkel Corporation patents that may cover such processes or compositions. We recommend that each prospective user test his proposed application before repetitive use, using this data as a guide. This product may be covered by one or more United States or foreign patents or patent applications.

### Trademark Usage

Except as otherwise noted, all trademarks in this document are trademarks of Henkel Corporation in the U.S. and elsewhere. ® denotes a trademark registered in the U.S. Patent and Trademark Office.

*(Provisional – awaiting legal clearance)* When this product is used to create a Regulated Medical Device, either the user assumes all responsibility to use this product only for Henkel supported and approved Indications for use or the user must take all responsibility to register their indication of use with the proper regulatory authority. Strict adherence to our information for use and validated production workflows (printer, washing, and post processing procedures), is critical in assuring a safe, biocompatible and effective printed appliance.



alphacam GmbH  
Erlenwiesen 16  
D-73614 Schorndorf  
Tel.: +49 7181 9222-0  
info@alphacam.de

alphacam austria GmbH  
Handelskai 92, Gate1 / 2. OG / Top A  
A-1200 Wien  
Tel.: +43 1 3619 600-0  
info@alphacam.at

alphacam swiss GmbH  
Zürcherstrasse 14  
CH-8400 Winterthur  
Tel.: +41 52 26207-50  
info@alphacam.ch



alphacam.de  
.at  
.ch